



Capnography for Nonintubated Patients: The Wave of the Future for Routine Monitoring of Procedural Sedation Patients

Debbie Sandlin, RN, CPAN

THE USE OF procedural sedation is growing dramatically because of the increase in performance of minimally invasive procedures in nonacute and acute care settings. As anesthesia agents have been refined to provide short-acting sedation with minimal side effects, procedural sedation is becoming increasingly desirable. Procedural sedation is not only commonly used in the operating room, but has many other applications such as endoscopy, radiology, cardiology, dentistry, physicians' offices, and pediatrics. The Joint Commission on Accreditation of Healthcare Organizations (JCAHO) defined 4 levels of sedation and anesthesia in January 2001.¹ These defined levels made clear that because sedation-to-anesthesia is a continuum, sedation patients should be monitored and treated the same as general anesthesia patients.

Table 1. Capnography Waveforms: Interpreting the Capnogram

A Capnogram is the graphical waveform depicting carbon dioxide (CO₂) concentration throughout respiration. End-tidal CO₂ (EtCO₂) refers to the measurement of carbon dioxide concentration at the end of exhalation. A normal range for EtCO₂ is 35–45 mmHg (4.5%–6%), similar to the range of CO₂ in arterial blood.

Key Terms:

- PaCO₂—Partial pressure of CO₂ in arterial blood
- EtCO₂—End-tidal carbon dioxide: measurement of the concentration of CO₂ at the end of exhalation
- Capnometry—Measurement and numerical display of CO₂ concentration at the patient's airway
- Capnography—Measurement and waveform display of CO₂ concentration in the patient's airway
- Capnogram—Waveform display of CO₂ throughout respiration

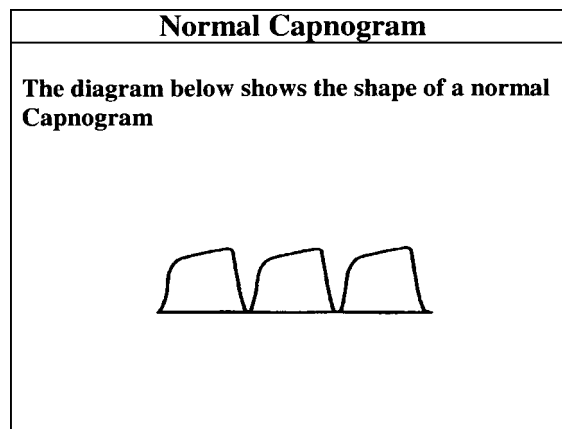


Fig 1. Normal capnogram. Reprinted with permission from Oridion Microstream Capnography Pocket Guide, page 21.

Capnography is the continuous measurement and display of carbon dioxide (CO₂) concentration in exhaled breath. A capnogram is the graphical waveform depicting CO₂ concentration throughout respiration (Table 1). A normal capnogram has a near zero baseline with a sharp rapid rise, a plateau, then a sharp rapid down shift (Fig 1). Abnormal capnograms occur for a multitude of reasons and present with varying changes from the normal (Fig 2).

Debbie Sandlin, RN, CPAN, is the Clinical Coordinator for the PACU and Presurgical Holding Unit at Southern Hills Medical Center, Nashville, TN.

Address correspondence to Debbie Sandlin, RN, CPAN, 508 Michele Dr, Antioch, TN 37013.

© 2002 by American Society of PeriAnesthesia Nurses.

1089-9472/02/1704-0009\$35.00/0

doi:10.1053/jpan.2002.34336











Abnormal Capnograms	
<p>Gradually Increasing EtCO₂</p>  <p>Possible causes:</p> <ul style="list-style-type: none"> • Hypoventilation • Malignant Hyperthermia • Rising body temperature • Increased metabolism • Partial airway obstruction • Absorption of CO₂ from exogenous source 	<p>Rise in Baseline and EtCO₂</p>  <p>Possible causes:</p> <ul style="list-style-type: none"> • Defective exhalation valve • Rebreathing of previously exhaled CO₂ • Exhausted CO₂ absorber
<p>Exponential Decrease in EtCO₂</p>  <p>Possible causes:</p> <ul style="list-style-type: none"> • Cardiopulmonary arrest • Pulmonary embolism • Sudden hypotension; massive blood loss • Cardiopulmonary bypass 	<p>Cardiogenic Oscillations</p>  <p>Causes: Cardiogenic oscillations are caused by changes in thoracic volume secondary to expansion and contraction of the myocardium with each heartbeat. They are usually seen in patients with small tidal volumes and slow respiratory rates, and are of little physiologic consequence.</p>
<p>Sudden Decrease in EtCO₂ to low, non-zero value</p>  <p>Possible causes:</p> <ul style="list-style-type: none"> • Leak in the airway system • ET tube in hypopharynx • Poorly fitting anesthetic mask • Partial airway obstruction • Partial disconnect from ventilator circuit 	<p>Spontaneous Breathing during mechanical ventilation</p>  <p>Causes: Spontaneous breathing efforts may be evident on the CO₂ waveform display. The patient on the top demonstrates poorer quality spontaneous breathing effort than the patient on the bottom.</p>
<p>Sudden loss of EtCO₂ to zero or near zero</p>  <p>Possible causes:</p> <ul style="list-style-type: none"> • Airway disconnection • Dislodged ET tube/esophageal intubation • Totally obstructed/kinked ET tube • Complete ventilator malfunction 	<p>Sustained low EtCO₂ without alveolar plateau</p>  <p>Possible causes:</p> <ul style="list-style-type: none"> • Incomplete exhalation • Partially kinked ET tube • Bronchospasm • Mucous plugging • Poor sampling techniques
<p>Sustained low EtCO₂ with good alveolar plateau</p>  <p>Possible causes:</p> <ul style="list-style-type: none"> • Hyperventilation • Hypothermia • Sedation, anesthesia • Dead space ventilation 	<p>Elevated EtCO₂ with good alveolar plateau</p>  <p>Possible causes:</p> <ul style="list-style-type: none"> • Inadequate minute ventilation/hypoventilation • Respiratory-depressant drugs • Hyperthermia, pain, shivering

Fig 2. Abnormal capnograms. Reprinted with permission from Oridion Microstream Capnography Pocket Guide, pages 22–25.

Capnographs currently are used to monitor ventilator status, airway leaks, ventilator circuit disconnects, and the early onset of malignant hyperthermia in intubated ventilated patients. During procedural sedation, capnography can be used to detect hypoventilation caused by sedation or narcot-

ics and monitor adequacy of ventilation. Current literature supports the use of capnography in the emergency room and intensive care units during procedural sedation for all ages,^{2,3} and capnography is being used more frequently in pediatric dentistry⁴ and in pediatric intensive care units.⁵

Patient Interfaces Smart CapnoLine®

- Easy to use: All one piece
- Oral or Nasal breathing
- Low Flow O₂

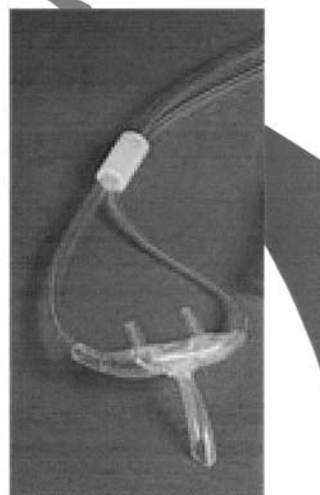



Fig 3. Oridion Smart CapnoLine divided cannula. Supplied by Oridion, with permission.

Although capnography does not eliminate the need for arterial blood gas sampling, when properly used it has the potential to reduce the frequency of some invasive procedures while

still providing valuable information.⁶ It certainly has implications for greater use in procedural sedation cases and may well become a standard of care in monitoring for procedural sedation.

New! Smart CapnoLine™ O₂

O₂/CO₂ – Oral/Nasal Cannula

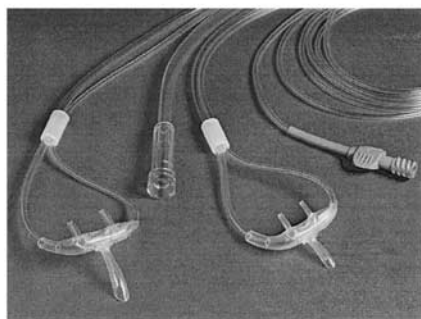

- Unique O₂ delivery provides greater comfort and reduces CO₂ sample dilution
- Uni-junction™ cannula samples only where breath is exhaled

Fig 4. Oridion Smart CapnoLine CO₂ sampling solution for nonintubated patients. Supplied by Oridion, with permission.

Oridion Systems (Jerusalem, Israel) has developed the Smart Capnoline O₂, which is the first system to display an accurate waveform display of exhaled CO₂ from sedated, nonintubated patients while delivering supplemental oxygen.⁷ This system displays the earliest possible warning signs of potentially fatal adverse events that may develop as a result of procedural sedation including airway obstruction, ventilatory depression, and apnea.

The Oridion Smart Capnoline uses a special cannula that is capable of measuring exhaled CO₂ from both the nose and mouth, while delivering supplemental oxygen (Fig 3). Very tiny holes are used to disperse a cloud of oxygen toward the nose and mouth while reducing CO₂ sampling dilution to a minimum (Fig 4). According to studies by Loughnan et al,⁸ the divided nasal cannula more accurately reflects end tidal CO₂ partial pressure and provides a more representative waveform when compared with a traditional facemask system, while delivering adequate supplemental oxygenation. Other studies conclude that the microstream capnometer provides a more accurate end tidal CO₂ partial pressure measurement in nonintubated, spontaneously breathing patients than conventional sidestream capnometers (Fig 5).^{9,10} This system provides crisp, clear waveforms and requires no routine calibration. It eliminates the problem that conventional mainstream capnometers have with excess moisture collection by using a special in-line filter.

This Oridion product is compatible with most monitoring systems, including (but not limited to) Datascope (Paramus, NJ), Datex Ohmeda (Madison, WI), Agilent Technologies-Phillips Medical Systems-Hewlett-Packard (Bathel, WA),

Smart CapnoLine™ O₂

The CO₂ sampling solution for non-intubated patients

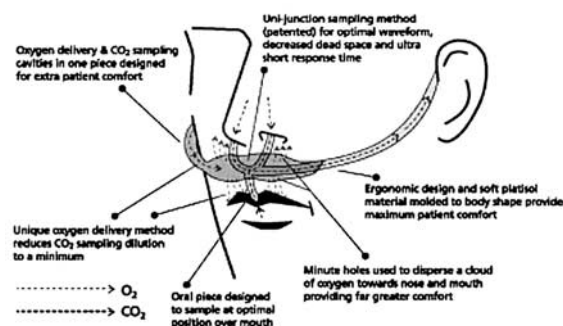


Fig 5. Interpreting the capnogram. Reprinted with permission from Oridion Microstream Capnography Pocket Guide, page 20.

Thermo Respiratory Group-Medical Data Electronics (Arleta, CA), Medtronic PhysioControl (Seattle, WA), Nellcor Puritan Bennett (Pleasanton, CA), and Novamatrix Medical (Wallingford, CT).

Standards for basic anesthetic monitoring developed by the American Society of Anesthesiologists (ASA) state that every patient receiving general anesthesia shall have continued monitoring for the presence of expired CO₂ unless invalidated by the nature of the patient, procedure, or equipment.¹¹ Now that an accurate and easy method for measurement of expired CO₂ in nonintubated, sedated patients exists, one can reasonably assume that these ASA standards may eventually be applied to procedural sedation patients to safeguard those patients who may cross the sedation-to-anesthesia continuum.

For additional information about this product, contact Oridion Medical Inc, 140 Town and Country Drive, Suite B, Danville, CA 94526, USA. 1-888-ORIDION or www.oridion.com.

References

1. Joint Commission on the Accreditation of Healthcare Organizations: Revisions to Anesthesia Care Standards Comprehensive Accreditation Manual for Hospitals effective January 1, 2001: Standards and Intents for Sedation and Anesthesia Care. Available at www.jcabo.org/standard/anesbap.html. Accessed January 16, 2002
2. Soubani AO: Noninvasive monitoring of oxygen and carbon dioxide. *Am J Emerg Med* 19:141-146, 2001
3. McQuillen KK, Steele DW: Capnography during sedation/analgesia in the pediatric emergency department. *Pediatr Emerg Care* 16:401-404, 2000
4. Wilson S, Farrell K, Griffen A, et al: Conscious sedation

experience in graduate pediatric dentistry programs. *Pediatr Dent* 23:307-314, 2001

5. Nadkarni UB, Shah AM, Desmukh CT: Non-invasive respiratory monitoring in paediatric intensive care unit. *J Postgrad Med* 46:149-152, 2000

6. St John RE, Thomson PD: Noninvasive respiratory monitoring. *Crit Care Nurs Clin North Am* 11:423-435, 1999

7. Press Release: Oridion receives FDA (Federal Drug Administration) clearance for novel monitoring device that provides earliest possible detection of respiratory adverse events that can occur during procedural sedation. Jerusalem, Israel, Nov 26, 2001

8. Loughnan TE, Monagle J, Copland JM, et al: A comparison of

carbon dioxide monitoring and oxygenation between facemask and divided nasal cannula. *Anesth Int Care* 28:151-154, 2000

9. Casati A, Gallioli G, Passaretta R, et al: End tidal carbon dioxide monitoring in spontaneously breathing, non-intubated patients. A clinical comparison between conventional side-stream and microstream capnometers. *Minerva Anesthesiol* 67:161-164, 2001

10. Casati A, Gallioli G, Scandroglio M, et al: Accuracy of end-tidal carbon dioxide monitoring using the NBP-75 microstream capnometer. A study in intubated ventilated and spontaneously breathing non-intubated patients. *Eur J Anaesthesiol* 17:622-666, 2000

11. American Society of Anesthesiologists: Standards for Basic Anesthetic Monitoring. Park Ridge, IL, ASA, 1977